

TEST REPORT



한국산업기술시험원
Korea Testing Laboratory

Report No. : 17-035982-02-2

Page of Pages : (1) / (2)



1. Client

Name : Join Medical Co., Ltd.

Address : 143-40, 3F, Gangdong-daero, Gangdong-gu, Seoul, Korea 05398

Date of Receipt : 2017. 06. 23.

2. Use of Report : For quality control

3. Test Sample

Description : AIR Sterilisation

Manufacturer : Novaerus (Ireland) Ltd.

Model Name : NV800

Serial Number : ***

Remark : ***

4. Date of Test : 2017. 06. 10. ~ 2017. 06. 14.

5. Test Standard/Method : KOUVA AS 01 : 2015

6. Testing Environment : Temperature : (23.0 ± 2.0) °C , Humidity : (50 ± 5) % R.H.

7. Test Results : Refer to the attached results

Note : 1. The test results contained apply only to the test sample(s) supplied by the client

2. This test report shall not be reproduced in full or in part without approval of the KTL in advance.

Affirmation	Tested by	 (Signature)	Technical Manager	 (Signature)
	Name : Lee, Jung-hoon		Name : JEON, Yong-Woo	

2017. 06. 26.

Korea Testing Laboratory



87, Digital-ro 26-gil, Guro-gu, Seoul, KOREA Tel.+82-2-860-1692 Fax. +82-2-860-1689

FP204-03-03



※ 위 마크는 추후 전자확인증 대조 프로그램에서 원본대조시 사용되는 2D코드입니다.

Test Results

1. Bacteria Test results

1) Results

Reference and Results Unit	Reference value	Results
AIR Sterilisation	over 60 %	83.8 %

2) Test unit

(1) Manufacture : Novaerus (Ireland) Ltd.


(2) Model Name : NV800

(3) Serial Number. : ***

3) Test Method and Conditions

Conditions Test method	Virus	Temp.	Humidity	Test chamber	Test time
KOUVA AS 01 : 2015, Air sterilizer	Phi-X174 (ATCC 13706-B1)	(23 ± 2) °C	(50 ± 5) % R.H.	60 m ³	30 min.

4) Photo of Unit

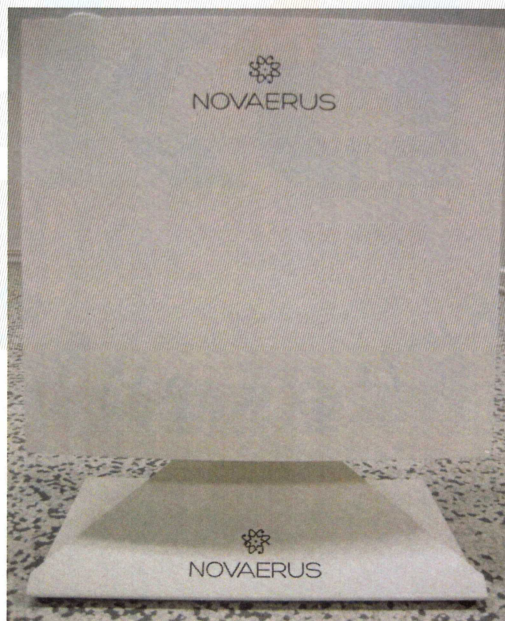

- End of document -

